

# Human/Monkey CCL11/Eotaxin ELISA Instructions

## Cat:EH0201

### Content

	CAT	Volume
① CP (Coated Plate)	EH0201CP	96 well
② S (Standard)	EH0201S,S1~S7,S0	9 vial
③ DA (Detect Antibody)	EH0201DA	6 ml/bottle
④ SH (Streptavidin-HRP)	ESH01	12 ml/bottle
⑤ AB (Assay Buffer 1×)	EAB01	12 ml/bottle
⑥ TS (TMB Substrate)	ETS01	12 ml/bottle
⑦ SS (Stop Solution)	ESS01	12 ml/bottle
⑧ WB (Wash Buffer 10×)	EWB01	50 ml/bottle
⑨ SF (Sealer Film)	ESF01	6 pieces

**NOTE:** After the kit is opened, the stabilization period of each content is 30 days, so please use the kit within 30 days after opening.

### REAGENT PREPARATION

#### Washing Buffer (1×) Preparation


Pour entire contents (50 ml) of the **Washing Buffer Concentrate** (10×) into a clean 500 ml graduated cylinder. Bring to final volume of 500 ml with glass-distilled or deionized water. Transfer to a clean wash bottle and store at 2 to 25°C.

#### Standard Curve Preparation:

S1 to S7 and S0 is ready to use for serum and plasma.

Other sample type, prepare the standard curve with whatever buffer (SPB, Sample Prepared Buffer) is used to prepare the sample, such as cell culture supernatant, tissue grinding liquid, cell lysate, etc. Urine sample use AB (Assay Buffer) prepare standard curve.

The human CCL11/Eotaxin Standard EH0201S 40000 pg/ml 30 μl + 270 μl SPB serves as the high standard (4000 pg/ml). Pipette 150 μl of SPB into each tube. Use the high standard to produce a 1:1 dilution series. Mix each tube thoroughly before the next transfer. SPB serves as the zero standard (0 pg/ml).

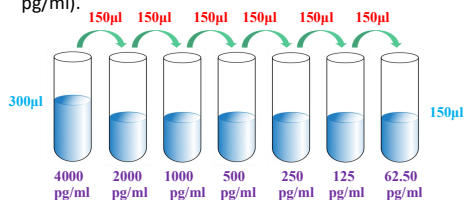


### ASSAY PROCEDURE

Bring all reagents and samples to room temperature before use.

- ① Prepare all reagents and working standards as directed in the previous sections.
- ② Remove excess **CP** (Coated Plate) strips from the plate frame, return them to the foil pouch and reseal.
- ③ Add 50 μl of **AB** (Assay Buffer) to each well.
- ④ Add 50 μl or 10 μl of **Standard or sample** per well. Ensure reagent addition is uninterrupted and completed within 15 minutes.
- ⑤ Add 50 μl of **DA** (Detect Antibody) to each well.
- ⑥ Cover with an **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 1 hour on a microplate **shaker** set at 500 rpm.
- ⑦ Aspirate each well and **wash**, repeating the process four times. Wash by filling each well with **WB** (Washing Buffer 300 μl). Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining **WB** (Washing Buffer) by aspirating or decanting. Invert the plate and **blot** it against clean paper towels.
- ⑧ Add 100 μl of **SH** (Streptavidin-HRP) to each well.
- ⑨ Cover with a new **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 30 min on a microplate **shaker** set at 500 rpm.
- ⑩ Repeat aspiration/**wash** as in step 7.
- ⑪ Add 100 μl of **TS** (TMB Substrate) to each well. Incubate for 5-30 minutes at room temperature.
- ⑫ Add 100 μl of **SS** (Stop Solution) to each well.
- ⑬ Determine the optical density within 30 minutes, using microplate **reader** set to 450 nm corrected with 570 nm or 630 nm.

## TYPICAL DATA

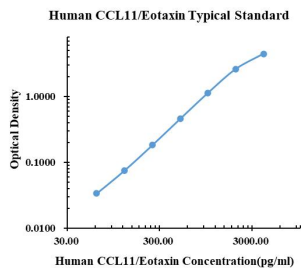

pg/ml	O.D.	Average	Corrected
0.00	0.0179	0.0182	0.0181
62.50	0.0510	0.0524	0.0517
125.00	0.0924	0.0940	0.0932
250.00	0.1999	0.2008	0.2004
500.00	0.4787	0.4712	0.4750
1000.00	1.1480	1.1570	1.1525
2000.00	2.7190	2.5540	2.6365
4000.00	4.4816	4.4996	4.4906

## SENSITIVITY

The minimum detectable dose (MDD) of human CCL11/Eotaxin is typically less than 4.73 pg/ml (50  $\mu$ l of sample volume) or 8.97 pg/ml (10  $\mu$ l of sample volume).

The MDD was determined by adding two standard deviations to the mean optical density value of ten zero standard replicates and calculating the corresponding concentration.

## PRECISION

**Intra-assay Precision (Precision within an assay)** Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.

**Inter-assay Precision (Precision between assays)**

Sample Number	Intra-assay Precision			Inter-assay Precision		
	S1	S2	S3	S1	S2	S3
22	22	22	22	6	6	6
Average (pg/ml)	111.0	495.8	1676.5	100.0	402.4	1352.0
Standard Deviation	6.2	23.4	93.6	4.1	19.1	74.6
Coefficient of Variation (%)	5.6	4.7	5.6	4.1	4.7	5.5

## RECOVERY

The spike recovery was evaluated by spiking 3 levels of human CCL11/Eotaxin into health human serum sample. The un-spiked serum was used as blank in this experiment.

The recovery ranged from 104% to 120% with an overall mean recovery of 117%.

## LINEARITY

To assess the linearity of the assay, five samples were spiked with high concentration of CCL11/Eotaxin in human serum and diluted with Sample Diluent to produce samples with values within the dynamic range of the assay.

The linearity ranged from 105% to 119% with an overall mean recovery of 116%.

## SAMPLE VALUES

Serum/Plasma – Thirty samples from apparently healthy volunteers and two samples from healthy monkeys were evaluated for the presence of human CCL11/Eotaxin in this assay. No medical histories

Sample Matrix	Sample Evaluated	Range (pg/ml)	Detectable %	Mean of Detectable (pg/ml)
Human Serum	30	n.d.-151.13	57	38.40
Monkey Serum	2	171.40-175.20	100	173.30

n.d. = non-detectable. Samples measured below the sensitivity are considered to be non-detectable.