

Mammalian CD62P/P-Selectin ELISA Instructions

Cat:EH0289

Content

	CAT	Volume
① CP (Coated Plate)	EH0289CP	96 well
② S (Standard)	EH0289S,S1~S7,S0	9 vial
③ SD (Sample Diluent)	ESD01	15 ml/bottle
④ DA-H (Detect Antibody-HRP 100×)	EH0289DA	50 µl/vial
⑤ DD (Detect Antibody Diluent)	EDD02	6 ml/bottle
⑥ SH (Streptavidin-HRP)	ESH01	12 ml/bottle
⑦ AB (Assay Buffer 1×)	EAB01	12 ml/bottle
⑧ TS (TMB Substrate)	ETS01	12 ml/bottle
⑨ SS (Stop Solution)	ESS01	12 ml/bottle
⑩ WB (Wash Buffer 10×)	EWB01	50 ml/bottle
⑪ SF (Sealer Film)	ESF01	6 pieces

NOTE: After the kit is opened, the stabilization period of each content is 30 days, so please use the kit within 30 days after opening.

Sample Dilution

Samples such as human and monkey serum 、 plasma require at least a 20-fold , mouse serum 、 plasma require at least a 200-fold, rat serum 、 plasma require at least a 100-fold dilution into Sample Diluent.


REAGENT PREPARATION

Standard Curve Preparation:

S1 to S7 and S0 is ready to use for serum and plasma.

Other sample type, prepare the standard curve with whatever buffer (SPB, Sample Prepared Buffer) is used to prepare the sample, such as cell culture supernatant, tissue grinding liquid, cell lysate, etc. Urine sample use AB (Assay Buffer) prepare standard curve.

The mammalian CD62P/P-Selectin Standard EH0289S 100000 pg/ml 30 µl + 270 µl SPB serves as the high standard (10000 pg/ml). Pipette 150 µl of SPB into each tube. Use the high standard to produce a 1:1 dilution series. Mix each tube thoroughly before the next transfer. SPB serves as the zero standard (0 pg/ml).

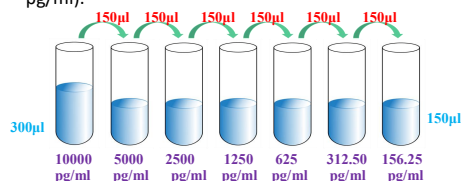

Washing Buffer (1×) Preparation

Pour entire contents (50 ml) of the **Washing Buffer Concentrate** (10×) into a clean 500 ml graduated cylinder. Bring to final volume of 500 ml with glass-distilled or deionized water. Transfer to a clean wash bottle and store at 2 to 25°C.

1×DA Preparation:

Mix well prior to making dilutions.


Make a 1:100 dilution of the concentrated Detect Antibody solution with **DD** (Detect Antibody Diluent) in a clean plastic tube as needed according to the Standards and Samples.

ASSAY PROCEDURE

Bring all reagents and samples to room temperature before use.

- ① Prepare all reagents and working standards as directed in the previous sections.
- ② Remove excess **CP** (Coated Plate) strips from the plate frame, return them to the foil pouch and reseal.
- ③ Add 50 µl of **AB** (Assay Buffer) to each well.
- ④ Add 50 µl or 10 µl of **Standard or sample** per well. Ensure reagent addition is uninterrupted and completed within 15 minutes.
- ⑤ Add 50 µl of **DA** (Detect Antibody) to each well.
- ⑥ Cover with an **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 1 hour on a microplate **shaker** set at 500 rpm.
- ⑦ Aspirate each well and **wash**, repeating the process four times. Wash by filling each well with WB (Washing Buffer 300 µl). Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining WB (Washing Buffer) by aspirating or decanting. Invert the plate and **blot** it against clean paper towels.
- ⑧ Add 100 µl of **SH** (Streptavidin-HRP) to each well.
- ⑨ Cover with a new **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 30 min on a microplate **shaker** set at 500 rpm.
- ⑩ Repeat aspiration/**wash** as in step 7.
- ⑪ Add 100 µl of **TS** (TMB Substrate) to each well. Incubate for 5-30 minutes at room temperature.
- ⑫ Add 100 µl of **SS** (Stop Solution) to each well.
- ⑬ Determine the optical density within 30 minutes, using microplate **reader** set to 450 nm corrected

TYPICAL DATA



pg/ml	O.D.	Average	Corrected
0.00	0.0444	0.0441	0.0443
156.25	0.1587	0.1492	0.1540
312.50	0.2757	0.2684	0.2721
625.00	0.4935	0.4962	0.4949
1250.00	0.8932	0.8620	0.8776
2500.00	1.4950	1.5650	1.4858
5000.00	2.3990	2.4770	2.3938
10000.00	3.3780	3.4450	3.3673

SENSITIVITY

The minimum detectable dose (MDD) of mammalian CD62P/P-Selectin is typically less than 8.19 pg/ml (50 μ l of sample volume) or 70.99 pg/ml (10 μ l of sample volume).

The MDD was determined by adding two standard deviations to the mean optical density value of ten zero standard replicates and calculating the corresponding concentration.

PRECISION

■ **Intra-assay Precision (Precision within an assay)** Three samples of known concentration were tested twenty-two times on one plate to assess intra-assay precision.

■ **Inter-assay Precision (Precision between assays)**

Sample Number	Intra-assay Precision			Inter-assay Precision		
	S1	S2	S3	S1	S2	S3
22	22	22	22	6	6	6
Average (pg/ml)	199.2	1022.8	3359.7	161.6	695.0	2182.5
Standard Deviation	10.0	44.6	381.0	7.6	29.3	104.0
Coefficient of Variation (%)	5.0	4.4	11.3	4.7	4.2	4.8

RECOVERY

The spike recovery was evaluated by spiking 3 levels of mammalian CD62P/P-Selectin into health mammalian serum sample. The un-spiked serum was used as blank in this experiment.

The recovery ranged from 80% to 115% with an overall mean recovery of 94%.

LINEARITY

To assess the linearity of the assay, five samples were spiked with high concentration of CD62P/P-Selectin in mammalian serum and diluted with Sample Diluent to produce samples with values within the dynamic range of the assay.

The linearity ranged from 80% to 112% with an overall mean recovery of 95%.

SAMPLE VALUES

Serum/Plasma – Thirty samples from apparently healthy volunteers, thirty samples from apparently healthy mice, thirty samples from apparently healthy rats and one sample from healthy monkeys were evaluated for the presence of mammalian CD62P/P-Selectin in this assay. No medical histories were available for the donors.

Sample Matrix	Sample Evaluated	Range (ng/ml)	Detectable %	Mean of Detectable (ng/ml)
Human Serum	30	7.85-29.14	100	18.17
Mouse Serum	30	355.11-903.67	100	572.82
Rat Serum	30	26.18-72.12	100	46.71
Monkey Serum	1	4.32	100	4.32

n.d. = non-detectable. Samples measured below the sensitivity are considered to be non-detectable.