

Human Lipoprotein A/LPA ELISA Instructions

Cat:EHY0171

Content

| | CAT | Volume |
|-----------------------------------|-----------------|--------------|
| 1 CP (Coated Plate) | EHY0171CP | 96 well |
| 2 S (Standard) | EHY0171S1~S7,S0 | 8 vial |
| 3 SD (Sample Diluent) | ESD01 | 15 ml/bottle |
| 4 DD (Detect Antibody Diluent) | EDD02 | 6 ml/bottle |
| 5 DA-H (Detect Antibody-HRP 100×) | EHY0171DA-H | 50μl/vial |
| 6 AB (Assay Buffer 1×) | EAB01 | 12 ml/bottle |
| 7 TS (TMB Substrate) | ETS01 | 12 ml/bottle |
| 8 SS (Stop Solution) | ESS01 | 12 ml/bottle |
| 9 WB (Wash Buffer 10×) | EWB01 | 50 ml/bottle |
| 10 SF (Sealer Film) | ESF01 | 6 pieces |

NOTE: After the kit is opened, the stabilization period of each content is 30 days, so please use the kit within 30 days after opening.

Sample Dilution

Samples such as serum、plasma require at least a 100-fold dilution into Sample Diluent. it is recommended to add 5 μl of sample + 495 μl of Sample Diluent.

REAGENT PREPARATION

Washing Buffer (1×) Preparation

Pour entire contents (50 ml) of the **Washing Buffer Concentrate (10×)** into a clean 500 ml graduated cylinder. Bring to final volume of 500 ml with glass-distilled or deionized water. Transfer to a clean wash bottle and store at 2 to 25°C.


1×DA Preparation:

Mix well prior to making dilutions.

Make a 1:100 dilution of the concentrated Detect Antibody solution with **DD** (Detect Antibody Diluent) in a clean plastic tube as needed according to the Standards and Samples.

Standard Curve Preparation:

S1 to S7 and S0 is ready to use for serum and plasma.

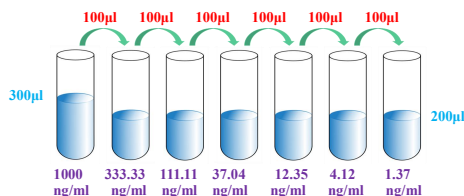

ASSAY PROCEDURE

Bring all reagents and samples to room temperature before use.

1 Prepare all reagents and working standards as directed in the previous sections.

2 Remove excess **CP** (Coated Plate) strips from the plate frame, return them to the foil pouch and reseal.

3 Add 50 μl of **AB** (Assay Buffer) to each well.

4 Add 10 μl of **Standard or sample** per well.

Ensure reagent addition is uninterrupted and completed within 15 minutes.

5 Add 50 μl of **DA-H** (Detect Antibody-HRP) to each well.

6 Cover with an **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 30 min on a microplate **shaker** set at 500 rpm.


7 Aspirate each well and **wash**, repeating the process four times. Wash by filling each well with **WB** (Washing Buffer 300 μl). Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining **WB** (Washing Buffer) by aspirating or decanting. Invert the plate and **blot** it against clean paper towels.

8 Add 100 μl of **TS** (TMB Substrate) to each well. Incubate for 5-30 minutes at room temperature.

9 Add 100 μl of **SS** (Stop Solution) to each well.

10 Determine the optical density within 30 minutes, using microplate **reader** set to 450 nm corrected with 570 nm or 630 nm.

TYPICAL DATA

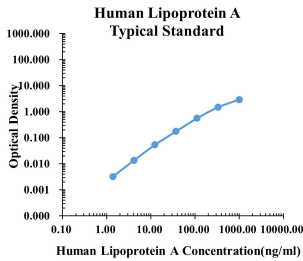

| ng/ml | O.D. | Average | Corrected |
|---------|--------|---------|-----------|
| 0.00 | 0.0050 | 0.0051 | 0.0051 |
| 1.37 | 0.0078 | 0.0088 | 0.0083 |
| 4.12 | 0.0202 | 0.0171 | 0.0187 |
| 12.35 | 0.0608 | 0.0575 | 0.0592 |
| 37.04 | 0.1870 | 0.1751 | 0.1811 |
| 111.11 | 0.5899 | 0.5499 | 0.5699 |
| 333.33 | 1.4950 | 1.5180 | 1.5065 |
| 1000.00 | 2.9860 | 2.8790 | 2.9325 |

SENSITIVITY

The minimum detectable dose (MDD) of human Lipoprotein A/LPA is typically less than 0.08 ng/ml (10 μ l of sample volume).

The MDD was determined by adding two standard deviations to the mean optical density value of ten zero standard replicates and calculating the corresponding concentration.

PRECISION

Intra-assay Precision (Precision within an assay) Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.

Inter-assay Precision (Precision between assays)

| | Intra-assay Precision | | | Inter-assay Precision | | |
|------------------------------|-----------------------|--------|--------|-----------------------|--------|--------|
| | S1 | S2 | S3 | S1 | S2 | S3 |
| Sample Number | 22 | 22 | 22 | 6 | 6 | 6 |
| Average (ng/ml) | 375.0 | 1408.8 | 3317.3 | 371.3 | 1405.8 | 3425.6 |
| Standard Deviation | 10.0 | 36.1 | 99.1 | 12.8 | 69.1 | 226.0 |
| Coefficient of Variation (%) | 2.7 | 2.6 | 3.0 | 3.4 | 4.9 | 6.6 |

RECOVERY

The spike recovery was evaluated by spiking 3 levels of human Lipoprotein A/LPA into health human serum sample. The un-spiked serum was used as blank in this experiment.

The recovery ranged from 87% to 118% with an overall mean recovery of 98%.

LINEARITY

To assess the linearity of the assay, five samples were spiked with high concentration of Lipoprotein A/LPA in human serum and diluted with Sample Diluent to produce samples with values within the dynamic range of the assay.

The linearity ranged from 91% to 117% with an overall mean recovery of 102%.

SAMPLE VALUES

Serum/Plasma – Thirty samples from apparently healthy volunteers were evaluated for the presence of human Lipoprotein A/LPA in this assay. No medical histories were available for the donors.

| Sample Matrix | Sample Evaluated | Range (ng/ml) | Detectable % | Mean of Detectable (ng/ml) |
|---------------|------------------|---------------|--------------|----------------------------|
| Serum | 30 | 65.60-8958.87 | 100 | 2085.89 |

n.d. = non-detectable. Samples measured below the sensitivity are considered to be non-detectable.