

# Human/Monkey Complement C3

## ELISA Instructions

**Cat:EHY0202**

### Content

	CAT	Volume
1 CP (Coated Plate)	EHY0202CP	96 well
2 S (Standard)	EHY0202S1	2 vial
3 SD (Sample Diluent)	ESD01	15 ml/bottle
4 DA-H (Detect Antibody-HRP 100×)	EHY0202DA-H	50 µl/vial
5 DD (Detect Antibody Diluent)	EDD02	6 ml/bottle
6 AB (Assay Buffer 1×)	EAB01	12 ml/bottle
7 TS (TMB Substrate)	ETS01	12 ml/bottle
8 SS (Stop Solution)	ESS01	12 ml/bottle
9 WB (Wash Buffer 10×)	EWB01	50 ml/bottle
10 SF (Sealer Film)	ESF01	6 pieces

**NOTE:** After the kit is opened, the stabilization period of each content is 30 days, so please use the kit within 30 days after opening.

### Sample Dilution

Samples such as serum, plasma require at least a 200-fold dilution into Sample Diluent. A suggested 200-fold dilution is 5 µl of sample + 995 µl of Sample Diluent.


### REAGENT PREPARATION

#### Standard Curve Preparation:

Reconstitute human/monkey Complement C3 Standard by addition of distilled water as S1. Reconstitution volume is stated on the label of the standard vial. Swirl or mix gently to insure complete and homogeneous solubilization (concentration of reconstituted standard = 50 µg/ml).

Allow the standard to reconstitute for 10-30 minutes. Mix well prior to making dilutions.

The human/monkey Complement C3 Standard EHY0202S1 as the high standard (50 µg/ml). Pipette 150 µl of SD (Sample Diluent) into each tube. Use the high standard to produce a 1:1 dilution series. Mix each tube thoroughly before the next transfer. SD (Sample Diluent) serves as the zero standard (0 µg/ml).

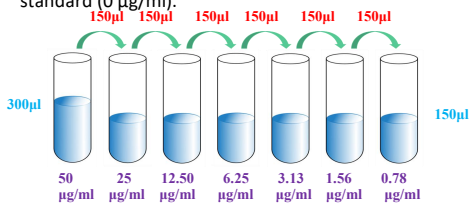

#### Washing Buffer (1×) Preparation

Pour entire contents (50 ml) of the **Washing Buffer Concentrate** (10×) into a clean 500 ml graduated cylinder. Bring to final volume of 500 ml with glass-distilled or deionized water. Transfer to a clean wash bottle and store at 2 to 25°C.

#### 1×DA Preparation:

Mix well prior to making dilutions.


Make a 1:100 dilution of the concentrated Detect Antibody solution with **DD** (Detect Antibody Diluent) in a clean plastic tube as needed according to the Standards and Samples.

### ASSAY PROCEDURE

Bring all reagents and samples to room temperature before use.

- 1 Prepare all reagents and working standards as directed in the previous sections.
- 2 Remove excess **CP** (Coated Plate) strips from the plate frame, return them to the foil pouch and reseal.
- 3 Add 50 µl of **AB** (Assay Buffer) to each well.
- 4 Add 10 µl of **Standard or sample** per well. Ensure reagent addition is uninterrupted and completed within 15 minutes.
- 5 Add 50 µl of **DA-H** (Detect Antibody-HRP) to each well.
- 6 Cover with an **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 30 min on a microplate **shaker** set at 500 rpm.
- 7 Aspirate each well and **wash**, repeating the process four times. Wash by filling each well with **WB** (Washing Buffer 300 µl). Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining **WB** (Washing Buffer) by aspirating or decanting. Invert the plate and **blot** it against clean paper towels.
- 8 Add 100 µl of **TS** (TMB Substrate) to each well. Incubate for 5-30 minutes at room temperature.
- 9 Add 100 µl of **SS** (Stop Solution) to each well.
- 10 Determine the optical density within 30 minutes, using microplate **reader** set to 450 nm corrected with 570 nm or 630 nm.

## TYPICAL DATA



µg/ml	O.D.	Average	Corrected
0.00	0.0079	0.0072	0.0076
0.78	0.0272	0.0261	0.0191
1.56	0.0599	0.0576	0.0512
3.13	0.1500	0.1343	0.1346
6.25	0.3914	0.3644	0.3704
12.50	0.9581	0.9236	0.9333
25.00	2.0780	2.1880	2.1255
50.00	3.1490	3.1720	3.1530

## SENSITIVITY

The minimum detectable dose (MDD) of human/monkey Complement C3 is typically less than 0.09 µg/ml (10 µl of sample volume).

The MDD was determined by adding two standard deviations to the mean optical density value of ten zero standard replicates and calculating the corresponding concentration.

## PRECISION

**Intra-assay Precision (Precision within an assay)** Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.

**Inter-assay Precision (Precision between assays)**

Sample Number	Intra-assay Precision			Inter-assay Precision		
	S1	S2	S3	S1	S2	S3
22	22	22	22	6	6	6
Average (µg/ml)	0.4	2.0	6.2	0.4	2.0	6.7
Standard Deviation	0.0	0.1	0.3	0.0	0.1	0.2
Coefficient of Variation (%)	4.9	4.1	4.6	4.0	3.4	3.3

## RECOVERY

The spike recovery was evaluated by spiking 3 levels of human/monkey Complement C3 into health human/monkey serum sample. The un-spiked serum was used as blank in this experiment.

The recovery ranged from 99% to 120% with an

## LINEARITY

To assess the linearity of the assay, five samples were spiked with high concentration of Complement C3 in human/monkey serum and diluted with Sample Diluent to produce samples with values within the dynamic range of the assay.

The linearity ranged from 102% to 115% with an overall mean recovery of 110%.

## SAMPLE VALUES

Serum/Plasma – Thirty samples from apparently healthy volunteers and two samples from healthy monkeys were evaluated for the presence of human/monkey Complement C3 in this assay. No medical histories were available for the donors.

Sample Matrix	Sample Evaluated	Range (mg/ml)	Detectable %	Mean of Detectable (mg/ml)
Human Serum	30	0.89-6.30	100	2.18
Monkey Serum	2	1.89-2.06	100	1.98

n.d. = non-detectable. Samples measured below the sensitivity are considered to be non-detectable.