

Mouse IL-1 beta Super Sensitivity ELISA Instructions

Cat:EMSS0029

Content

	CAT	Volume
① CP (Coated Plate)	EMSS0029CP	96 well
② S (Standard)	EMSS0029S,S1~S7,S0	9 vial
③ DA (Detect Antibody)	EMSS0029DA	6 ml/bottle
④ SH (Streptavidin-HRP)	ESHSS03	12 ml/bottle
⑤ AB (Assay Buffer 1×)	EAB01	12 ml/bottle
⑥ TS (TMB Substrate)	ETS01	12 ml/bottle
⑦ SS (Stop Solution)	ESS01	12 ml/bottle
⑧ WB (Wash Buffer 10×)	EWB01	50 ml/bottle
⑨ SF (Sealer Film)	ESF01	6 pieces

NOTE: After the kit is opened, the stabilization period of each content is 30 days, so please use the kit within 30 days after opening.

REAGENT PREPARATION

Washing Buffer (1×) Preparation


Pour entire contents (50 ml) of the **Washing Buffer Concentrate** (10×) into a clean 500 ml graduated cylinder. Bring to final volume of 500 ml with glass-distilled or deionized water. Transfer to a clean wash bottle and store at 2 to 25°C.

Standard Curve Preparation:

S1 to S7 and S0 is ready to use for serum and plasma.

Other sample type, prepare the standard curve with whatever buffer (SPB, Sample Prepared Buffer) is used to prepare the sample, such as cell culture supernatant, tissue grinding liquid, cell lysate, etc. Urine sample use AB (Assay Buffer) prepare standard curve.

The mouse IL-1 beta Standard EMSS0029S 1000 pg/ml 30 μ l + 270 μ l SPB serves as the high standard (100 pg/ml). Pipette 150 μ l of SPB into each tube. Use the high standard to produce a 1:1 dilution series. Mix each tube thoroughly before the next transfer. SPB serves as the zero standard (0 pg/ml).

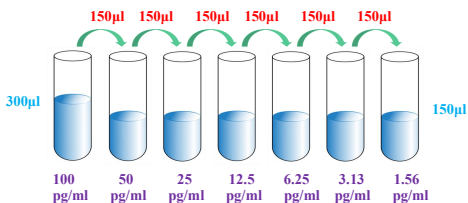

ASSAY PROCEDURE


Bring all reagents and samples to room temperature before use.

- ① Prepare all reagents and working standards as directed in the previous sections.
- ② Remove excess **CP** (Coated Plate) strips from the plate frame, return them to the foil pouch and reseal.
- ③ Add 50 μ l of **AB** (Assay Buffer) to each well.
- ④ Add 10 μ l or 50 μ l of **Standard or sample** per well. The volume of the sample added should be consistent with that of the standard. Ensure reagent addition is uninterrupted and completed within 15 minutes.
- ⑤ Add 50 μ l of **DA** (Detect Antibody) to each well.
- ⑥ Cover with an **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 1 hour on a microplate **shaker** set at 500 rpm.
- ⑦ Aspirate each well and **wash**, repeating the process four times. Wash by filling each well with **WB** (Washing Buffer 300 μ l). Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining **WB** (Washing Buffer) by aspirating or decanting. Invert the plate and **blot** it against clean paper towels.
- ⑧ Add 100 μ l of **SH** (Streptavidin-HRP) to each well.
- ⑨ Cover with a new **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 30 min on a microplate **shaker** set at 500 rpm.
- ⑩ Repeat aspiration/**wash** as in step 7.
- ⑪ Add 100 μ l of **TS** (TMB Substrate) to each well. Incubate the sample of 10 μ l at room temperature for about 20 minutes; incubate the sample of 50 μ l at room temperature for about 8 minutes.
- ⑫ Add 100 μ l of **SS** (Stop Solution) to each well.
- ⑬ Determine the optical density within 30 minutes, using microplate **reader** set to 450 nm corrected with 570 nm or 630 nm.

TYPICAL DATA


For every test, a standard curve must be established for each microplate.

Mouse IL-1 beta 10 μ l sample amount standard curve:



pg/ml	O.D.	Average	Corrected
0.00	0.1280	0.1360	0.1320
1.56	0.1530	0.1724	0.1627
3.13	0.1902	0.2052	0.1977
6.25	0.2792	0.2809	0.2801
12.50	0.4370	0.4454	0.4412
25.00	0.7625	0.7219	0.7422
50.00	1.3050	1.3190	1.3120
100.00	2.5070	2.4660	2.4865

Mouse IL-1 beta 50 μ l sample amount standard curve:



pg/ml	O.D.	Average	Corrected
0.00	0.0655	0.0606	0.0631
1.56	0.1368	0.1386	0.1377
3.13	0.2198	0.2308	0.2253
6.25	0.3742	0.3754	0.3748
12.50	0.6713	0.6800	0.6757
25.00	1.2790	1.2910	1.2850
50.00	2.2110	2.1960	2.2035
100.00	3.7030	3.5740	3.6385

SENSITIVITY

The minimum detectable dose (MDD) of mouse IL-1 beta with a 10 μ l sample is typically less than 0.36 pg/ml; with a 50 μ l sample is typically less than 0.12 pg/ml;

The MDD was determined by adding two standard deviations to the mean optical density value of ten zero standard replicates and calculating the corresponding concentration.

PRECISION

■ **Intra-assay Precision (Precision within an assay)** Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.

■ **Inter-assay Precision (Precision between**

Sample Number	Intra-assay Precision			Inter-assay Precision		
	S1	S2	S3	S1	S2	S3
22	22	22	22	6	6	6
Average (pg/ml)	1.8	9.7	29.2	1.8	9.7	29.4
Standard Deviation	0.1	0.5	1.3	0.1	0.5	1.4
Coefficient of Variation (%)	5.5	4.7	4.5	5.7	4.8	4.6

RECOVERY

The spike recovery was evaluated by spiking 3 levels of mouse IL-1 beta into health mouse serum sample. The un-spiked serum was used as blank in this experiment.

The recovery ranged from 81% to 111% with an overall mean recovery of 98%.

LINEARITY

To assess the linearity of the assay, five samples were spiked with high concentration of IL-1 beta in mouse serum and diluted with Sample Diluent to produce samples with values within the dynamic range of the assay.

The linearity ranged from 92% to 107% with an overall mean recovery of 99%.

SAMPLE VALUES

Serum/Plasma – Thirty samples from apparently healthy mice were evaluated for the presence of IL-1 beta in this assay. No medical histories were available for the donors.

Sample Matrix	Sample Evaluated	Range (pg/ml)	Detectable %	Mean of Detectable (pg/ml)
Serum	30	0.18-3.93	100	1.47